


**DATA SHEET-V1**  
**REMBRANDT® EGFR AMPLIFICATION**  
**FISH DETECTION**

Ref	<b>C816K.2030.05</b>		5 T
	<b>C816K.2030.10</b>		10 T

dextran sulphate and SSC) and are ready to use solutions.

**Intended use**

- I. The REMBRANDT® EGFR amplification FISH detection assay is an in-vitro diagnostics medical device intended for the detection of gene amplification of the locus 7p11.2 compared to copy numbers of chromosome 7 by means of *in situ* hybridization.
- II. The REMBRANDT® EGFR amplification FISH detection assay is intended for the detection of the locus 7p11.2 compared to copy numbers of chromosome 7 in fixed cells. The clinical interpretation of the results should not be established on the basis of a single test result. A precise diagnosis, in fact, should take into consideration clinical history, symptoms, as well as other possible test data.
- III. The REMBRANDT® EGFR amplification FISH detection assay kit is a quantitative assay for the detection of the locus 7p11.2 and chromosome 7 copy numbers.
- IV. The intended users are qualified laboratory employees in cytology and/or pathology. The product is intended for professional use.

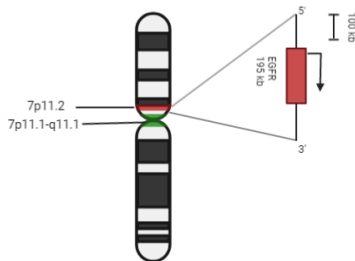

**Test principle**

In a fluorescent *in situ* hybridization assay, a double stranded DNA probe labelled with a fluorochrome is used. The labelled DNA probe is diluted in a hybridization mixture. The hybridization mixture containing the DNA probe is added to the specimen. A co-denaturation will ensure that the genomic DNA and the probe DNA become single stranded. After denaturation, the probe DNA is able to hybridize to its complementary target sequences in the cells. In the REMBRANDT® EGFR amplification assay, the fluorochrome is attached to the probe and the signals can be visualized directly by fluorescent microscopy after hybridization.

**Clinical relevance**

On the chromosome 7, locus p11.2, the gene for the Epidermal Growth Factor Receptor (EGFR), also known as HER1, is a tyrosine kinase receptor type 1 is located. EGFR is able to interact with epidermal growth factor proteins which result in proliferation. Increased activity of EGFR can result in proliferative diseases such as non-small-cell lung carcinoma (80-85% of all lung cancers). Moreover, EGFR amplifications have been associated with lung adenocarcinoma, glioblastoma, colon adenocarcinoma and breast carcinoma (Yoo et al., 2010).

**Reagents provided**

Product name	Product number	Amount
Labelled probe (depending on label and size choice)		
●EGFR amplification -FISH probes orange/ green detection	C816P.2030.05	5 T
●EGFR amplification -FISH probes orange/ green detection	C816P.2030.10	10 T
Pepsin powder	R011R.0000	1 g
Pepsin diluent	R018R.0000	15 ml
PanWash 4, 25X SSC	R025R.0000	15 ml
Fluorescent Mounting medium	Z000R.0050	1 ml

**Probe specification**

The EGFR amplification probes set consists of a 600 kb probe detecting the 7p11.2 locus and a 0.68 kb centromeric probe detecting the centromeric region of chromosome 7. The centromeric region is detected by green fluorescence (AF488) and the locus is detected by orange fluorescent detection (AF555). The EGFR amplification probe is able to completely cover the EGFR gene with flanking sequences on the 5' and 3' of the gene for signal enhancement. The EGFR amplification probes are pre-mixed in a hybridization mixture (formamide,

## Assay procedure

REMBRANDT® EGFR amplification FISH detection assay procedure for cytological specimen.

- I. Incubate slides in pre-heated proteolytic work solution (prepare according to section 1.9 of Manual-FISH) (R011R.000 + R018R.000) at 37 °C (100 µg/ml) for 15 minutes followed by a brief rinsing in 0.01M HCl (1x 2 minutes) and subsequent rinses in PBS (2x 1 minute)
- II. Flush wash slides in deionised water, followed by dehydration in graded ethanol series (ethanol 70%, 96%, 96%, 100%, 100%) 1 minute each and air-dry slides for 15 minutes

**Do not treat more than 5 slides at the same time, because the temperature of the pre-heated solutions may drop dramatically, thus causing incomplete pre-treatment. Additionally, allow the slides to air-dry as recommended; otherwise sections will be lost.**

- III. Homogenize probe solution (C816P.2030.YY) a spin briefly. Apply 15 µl of probe solution to each specimen. Cover all specimens with a cover slip (avoid air bubbles). Denature slides on a 80 °C hotplate or other heating device for 3 minutes

**Work in a pre-set order to ensure that all slides have been incubated at 80 °C for the exact same time. Do not denature more than 5 slides at the same time, the temperature of the heating device may drop dramatically, thus causing incomplete denaturation.**

- IV. Transfer the slides into a moist environment and incubate for 16 hours at 37 °C.
- V. Remove coverslips by soaking the slides in PBS at room temperature
- VI. Incubate the slides in diluted, pre-heated PanWash 4 (R025R.000) (prepare according to section 1.9 of Manual-FISH)


**Do not incubate more than 5 slides at the same time in PanWash 4, the temperature of the PanWash 4 may drop dramatically, causing wrong stringency conditions.**

- VII. Incubate the slides in PBS at room temperature for 1 minute
- VIII. Dehydrate the slides in graded ethanol series (70%, 96%, 96%, 100%, 100%) 1 minute each and air-dry the slides for 15 minutes (in the dark)
- IX. Mount the slides by applying mounting medium (Z000R.0050) and coverslip

## Interpretation of results

Hybridization of the EGFR amplification probe is viewed using a fluorescence microscope equipped with appropriate excitation and emission filters for orange detection:  $\lambda_{exc}$  555 nm,  $\lambda_{em}$  572 nm. Allowing visualization of orange fluorescent signal concentrated at the 7p11.2 locus of chromosome 7 in combination with green fluorescent signals representing the centromeric region of chromosome 7. The enumeration EGFR copy numbers of conducted by microscopic examination of interphase nuclei, compared to the signals representing chromosome 7. The fluorescently-stained locus of chromosome 7 stand out brightly against the general fluorescence of the nucleus. The EGFR amplification procedure enables visual enumeration of copy numbers of the 7p11.2 locus compared to chromosome 7 copy numbers within the nuclei. Enumerate the fluorescent signals in the interphase nucleus using a 40X or 63X magnification. Objectives with higher magnification (eg, 63X or 100X) should be used to verify or resolve questions about split or diffused signals. Enumerate at least 100 nuclei per slide for accurate analysis.

- Two signals in close proximity and approximately the same sizes but not connected by a visible link are counted as 2 signals.
- Count a diffuse signal as 1 signal if diffusion of the signal is contiguous and within an acceptable boundary.
- Two small signals connected by a visible link are counted as 1 signal.
- Enumerate the number of nuclei with 0, 1, 2, 3, 4, or >4 signals. Count nuclei with 0 signals only if there are other nuclei with at least 1 signal present in the field of view. If the accuracy of the enumeration is in doubt, repeat the enumeration in another area of the slide.
- Do not enumerate nuclei with uncertain signals (Arsham et al., 2017)

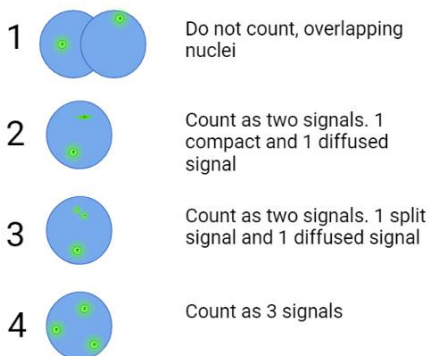

The EGFR amplification FISH assay is reported as positive if at least 40% of the scored cells contain  $\geq 4$  copies of the EGFR gene (locus 7p11.2) or in cases of gene amplification. Gene amplification can be characterised as:

- A ratio of EGFR/CEP7 copy numbers of at least  $\geq 2.00$  in all scored nuclei
- If a gene cluster of at least  $\geq 4$  signals is present in  $\geq 10\%$  of the assessed cells
- If at least 15 copies of EGFR signals are present in  $\geq 10\%$  of the assessed cells

## Performance characteristics

### Analytical Sensitivity and Specificity

The analytical sensitivity and specificity were investigated within PanPaths analytical performance assessment. Precision was investigated for the EGFR amplification assay and results are available upon request.

### Analytical sensitivity

The analytical sensitivity was determined in three levels. The normal cut-off percentage was determined based on assessment of 200 individual nuclei in two samples of healthy interphase lymphocytes from peripheral blood. The beta inversion was used to determine the percentage of normal-cut off. For the noise-to-signal percentage, the noise and signal values were determined for 100 signals in interphase lymphocytes from peripheral blood of two independent samples. The differences between noise and signal were evaluated using a 95% confidence interval. For the hybridization efficiency, 200 individual nuclei were assessed for the presence of FISH signals.

Performance characteristic	Outcome
Normal cut-off percentage	10.9%
Noise-to-signal cut-off percentage	14.8%
Hybridization efficiency	98.5%

### Analytical specificity

The analytical specificity was determined in two levels. The theoretical specificity was determined by sequencing analysis of the probe DNA and mapping on Hg38. The practical specificity was determined by assessing the hybridization pattern in metaphase chromosomes of interphase lymphocytes from peripheral blood.

Performance characteristic	Outcome
Theoretical specificity	Mapped on chromosome the locus 7p11.2 and the centromeric region 7p11.1-q11.1
Practical specificity	100%

## Limitations of Procedure

- The REMBRANDT® EGFR amplification FISH assay is solely applicable for the detection locus 7p11.2, which may be present in cell preparations (cytological specimen i.e. interphase lymphocytes from peripheral blood samples).
- Either human tissue sections or human cytological preparations may be used. Samples must be fixed in buffered formalin or alcohol. In tissue sections are required, the sections should be prepared in a 4  $\mu$ m thickness. Furthermore, the tissues should be glued to the glass slides with a bio-adhesive (e.g. organ silane), dried at room temperature, subsequently dried at 37 °C overnight and lastly completely deparaffinized in xylene and alcohol series and air dried.
- Cytological specimen should be prepared as required by the user, fixed with cytological fixation agent, rinsed in distilled water prior to the ISH procedure and air dried.
- Many factors can influence the performance of the ISH procedure. Failure in detection can be due to i.e. improper sampling, handling, the time lapse between tissue removal and fixation, the size of the tissue specimen in the fixation medium, the fixation time, processing fixed tissue, the thickness of the section, the bio-adhesive on the slide, deparaffinisation procedure, incubation times, proteolytic pre-treatment, detection reagents, incubation temperatures and interpretation of results.
- The performance of the ISH procedure is also affected by the sensitivity of the method and the presence of the locus 7p11.2 and the centromeric region of chromosome 7. In case the limit of the sensitivity is reached a false negative reaction may be the result.
- The REMBRANDT® EGFR amplification FISH assay results should not be relied on in case the sampling, sampling method, sample quality, sample preparation, reagents used, controls and procedure followed are not optimal or as described the working protocols.
- The clinical interpretation of the results should not be established on the basis of a single test result. A precise diagnosis should take into consideration clinical history as well as data obtained from other molecular test (i.e. WGS).
- Therapeutic considerations based on the result of this test alone should not be taken. Results should be verified by other traditional diagnostic methods such as but not limited to clinical history, symptoms, as well as morphological data.
- The medical profession should be aware of risks and factors influencing the fluorescent signal intensity while interpreting the test result. Microscopy settings might influence the signal intensity and/or interpretation.
- Laboratory personnel performing the test should be trained and knowledgeable to be able to interpret the test results.

## Storage and handling

Store kit and its contents at 2-8°C. Store the dissolved and aliquoted reagents at recommended temperatures. When used and stored as indicated, the kit is stable until the expiry date printed on the box.

Product	Product number	Storage conditions
EGFR/CEP7 Probe orange /green detection Pepsin powder	C816P.XXXX  R011R.0000	2-8 °C  Powder: 2-25°C, ambient temperature
Pepsin diluent	R018R.0000	Dissolved: -20°C Concentrated solution and diluted: 2-25°C, ambient temperature
PanWash 4, 25X SSC	R025R.0000	Concentrated solution and diluted: 2-25°C, ambient temperature
Fluorescent mounting medium	Z000R.0050	2-8 °C



## Hazard statements

H315 - Causes skin irritation  
H319 - Causes serious eye irritation  
H351 - Suspected of causing cancer  
H360D - May damage the unborn child  
H373 - May cause damage to organs through prolonged or repeated exposure

## Precautionary Statements

P202 - Do not handle until all safety precautions have been read and understood  
P280 - Wear protective gloves/protective clothing/eye protection/face protection  
P302 + P352 - IF ON SKIN: Wash with plenty of water and soap  
P305 + P351 + P338 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing  
P308 + P313 - IF exposed or concerned: Get medical advice/attention  
P362 + P364 - Take off contaminated clothing and wash it before reuse  
P405 - Store locked up

## Additional information

### Product in combination with other devices

The REMBRANDT® DNA probes are intended for stand-alone usage. The in vitro diagnostic is intended to be used in combination with standard cytological preparation

methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature and incubation time control(s), proteolytic-, detection- and other reagents (not supplied with this reagent) and a microscope. The combination has been tested and validated. Since the standard cytological preparation methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature controls, incubation time control(s) and other not supplied reagents such as but not limited to proteolytic reagents, detection reagents and a microscope is not combined with the device as a product, conformity with the essential requirements is not applicable. Assay validation criteria are mentioned in 'Interpretation of the Results' and are also depending on clinical state of the sample, which may influence the validation criteria.

For additional information regarding the REMBRANDT® assays, a manual is included which specifies the following subjects:

- Controls
- Materials required but not included
- Storage and shelf-life
- Performance precautions
- Preparations of reagents
- Specimen collection
- Quality control
- Trouble shooting guide

## Technical assistance

For technical assistance regarding the products performance, please contact [info@panpath.nl](mailto:info@panpath.nl) or call +31 495499090. Visit our website for reprints of datasheets or additional documentation. [www.panpath.nl](http://www.panpath.nl)

## Literature list

- Arsham, M. S., Barch, M. J., & Lawce, H. J. (2017). *The AGT Cytogenetics Laboratory Manual The AGT Cytogenetics Laboratory Manual Edited by* (Vol. 4).
- Yoo, S. B., Lee, H. J., Park, J. O., Choe, G., Chung, D. H., Seo, J. W., & Chung, J. H. (2010). Reliability of chromogenic in situ hybridization for epidermal growth factor receptor gene copy number detection in non-small-cell lung carcinomas: A comparison with fluorescence in situ hybridization study. *Lung Cancer*, 67(3), 301–305. <https://doi.org/10.1016/j.lungcan.2009.05.002>

**DATA SHEET-V1**  
**REMBRANDT® LSI 7p11.2/CEP7-**  
**FISH DETECTION**

RUO

**Pan**  
**Path**

Ref	C816K.2030.05		5 T
	C816K.2030.10		10 T

**Intended use**


- I. The REMBRANDT® LSI 7p11.2/CEP7-FISH detection assay is for research use only and is intended for the 7p11.2 locus, compared to the centromeric region of chromosome 7 by means of *in situ* hybridization.
- II. The REMBRANDT® LSI 7p11.2/CEP7-FISH detection assay is intended for the detection of the 7p11.2 locus, compared to the centromeric region of chromosome 7 in fixed cells. A clinical diagnosis should not be established based on the performance of this test.
- III. The intended users are qualified laboratory employees in cytology and/or pathology. The product is intended for professional use.

**Clinical relevance**

On the chromosome 7, locus p11.2, the gene for the Epidermal Growth Factor Receptor (EGFR), also known as HER1, is a tyrosine kinase receptor type 1 is located. EGFR is able to interact with epidermal growth factor proteins which result in proliferation. Increased activity of EGFR can result in proliferative diseases such as non-small-cell lung carcinoma (80-85% of all lung cancers). Moreover, EGFR amplifications have been associated with lung adenocarcinoma, glioblastoma, colon adenocarcinoma and breast carcinoma (Yoo et al., 2010).

**Probe specification**

The LSI 7p11.2/CEP7 probe set consists of a 600 kb probe detecting the 7p11.2 locus and a 0.68 kb centromeric probe detecting the centromeric region of chromosome 7. The centromeric region is detected by green fluorescence (AF488) and the locus is detected by orange fluorescent detection (AF555). The LSI 7p11.2 probe is able to completely cover the EGFR gene with flanking sequences on the 5' and 3' of the gene for signal enhancement. The LSI 7p11.2/CEP7 probes are pre-mixed in a hybridization mixture (formamide, dextran sulphate and SSC) and are ready to use solutions.

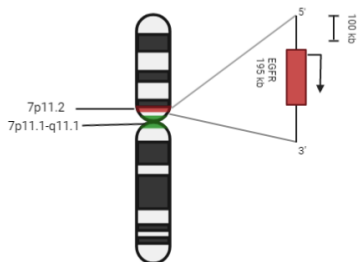

**Test principle**

In a fluorescent *in situ* hybridization assay, a double stranded DNA probe labelled with a fluorochrome is used. The labelled DNA probe is diluted in a hybridization mixture. The hybridization mixture containing the DNA probe is added to the specimen. A co-denaturation will ensure that the genomic DNA and the probe DNA become single stranded. After denaturation, the probe DNA is able to hybridize to its complementary target sequences in the cells. In the REMBRANDT® LSI 7p11.2/CEP7-FISH assay, the fluorochrome is attached to the probe and the signals can be visualized directly by fluorescent microscopy after hybridization.

**Reagents provided**

Product name	Product number	Amount
Labelled probes (depending on label and size choice)		
● LSI 7p11.2/CEP7-FISH probes orange/green detection	C816P.2030.05	5 T
● LSI 7p11.2/CEP7-FISH probes orange/green detection	C816P.2030.10	10 T
Pepsin powder	R011R.0000	1 g
Pepsin diluent	R018R.0000	15 ml
PanWash 4, 25X SSC	R025R.0000	15 ml
Fluorescent Mounting medium	Z000R.0050	1 ml

## Assay procedure

REMBRANDT® LSI 7p11.2/CEP7-FISH detection assay procedure for cytological specimen.

- I. Incubate slides in pre-heated proteolytic work solution (prepare according to section 1.9 of Manual-FISH) (R011R.000 + R018R.000) at 37 °C (100 µg/ml) for 15 minutes followed by a brief rinsing in 0.01M HCl (1x 2 minutes) and subsequent rinses in PBS (2x 1 minute)
- II. Flush wash slides in deionised water, followed by dehydration in graded ethanol series (ethanol 70%, 96%, 96%, 100%, 100%) 1 minute each and air-dry slides for 15 minutes

**Do not treat more than 5 slides at the same time, because the temperature of the pre-heated solutions may drop dramatically, thus causing incomplete pre-treatment. Additionally, allow the slides to air-dry as recommended; otherwise sections will be lost.**

- III. Homogenize probe solution (C816P.2030.YY) a spin briefly. Apply 15 µl of probe solution to each specimen. Cover all specimens with a cover slip (avoid air bubbles). Denature slides on a 80 °C hotplate or other heating device for 3 minutes

**Work in a pre-set order to ensure that all slides have been incubated at 80 °C for the exact same time. Do not denature more than 5 slides at the same time, the temperature of the heating device may drop dramatically, thus causing incomplete denaturation.**

- IV. Transfer the slides into a moist environment and incubate for 16 hours at 37 °C.
- V. Remove coverslips by soaking the slides in PBS at room temperature
- VI. Incubate the slides in diluted, pre-heated PanWash 4 (R025R.000) (prepare according to section 1.9 of Manual-FISH)

**Do not incubate more than 5 slides at the same time in PanWash 4, the temperature of the PanWash 4 may drop dramatically, causing wrong stringency conditions.**


- VII. Incubate the slides in PBS at room temperature for 1 minute
- VIII. Dehydrate the slides in graded ethanol series (70%, 96%, 96%, 100%, 100%) 1 minute each and air-dry the slides for 15 minutes (in the dark)
- IX. Mount the slides by applying mounting medium (Z000R.0050) and coverslip

## Interpretation of results

Hybridization of the LSI 7p11.2/CEP7 probes is viewed using a fluorescence microscope equipped with appropriate excitation and emission filters for orange detection:  $\lambda_{exc}$  555 nm,  $\lambda_{em}$  572 nm. Allowing visualization of orange fluorescent signal concentrated at the p11.2 locus of chromosome 7 in combination with green fluorescent signals representing the centromeric region of chromosome 7.

The assay procedure enables visual enumeration of the 7p11.2 locus compared to the centromeric region of chromosome 7 within the nuclei. Enumerate the fluorescent signals in the interphase nucleus using a 40X or 63X magnification. Objectives with higher magnification (eg, 63X or 100X) should be used to verify or resolve questions about split or diffused signals. Enumerate at least 100 nuclei per slide for accurate analysis.

- Two signals in close proximity and approximately the same sizes but not connected by a visible link are counted as 2 signals.
- Count a diffuse signal as 1 signal if diffusion of the signal is contiguous and within an acceptable boundary.
- Two small signals connected by a visible link are counted as 1 signal.
- Enumerate the number of nuclei with 0, 1, 2, 3, 4, or >4 signals. Count nuclei with 0 signals only if there are other nuclei with at least 1 signal present in the field of view. If the accuracy of the enumeration is in doubt, repeat the enumeration in another area of the slide.
- Do not enumerate nuclei with uncertain signals (Arsham et al., 2017)

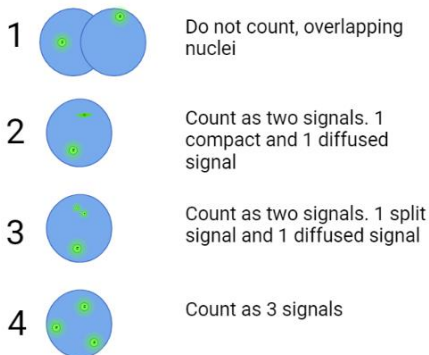

## Performance characteristics

### Analytical Sensitivity and Specificity

The LSI 7p11.2/CEP7-FISH detection assay was analytically validated for LSI 7p11.2/CEP7-FISH detection. The results of the direct fluorescent assay are shown. However, for the REMBRANDT® LSI 7p11.2/CEP7-FISH detection assay, the detection system may influence the performance characteristics and LSI 7p11.2/CEP7-FISH detection assay in combination with different detection systems should be evaluated carefully by the end-user.

### Analytical sensitivity

The analytical sensitivity was determined in three levels. The normal cut-off percentage was determined based on assessment of 200 individual nuclei in two samples of healthy interphase lymphocytes from peripheral blood. The beta inversion was used to determine the percentage of normal-cut off. For the noise-to-signal percentage, the noise and signal values were determined for 100 signals in interphase lymphocytes from peripheral blood of two independent samples. The differences between noise and signal were evaluated using a 95% confidence interval. For the hybridization efficiency, 200 individual nuclei were assessed for the presence of FISH signals.

Performance characteristic	Outcome
Normal cut-off percentage	10.9%
Noise-to-signal cut-off percentage	14.8%
Hybridization efficiency	98.5%

### Analytical specificity

The analytical specificity was determined in two levels. The theoretical specificity was determined by sequencing analysis of the probe DNA and mapping on Hg38. The practical specificity was determined by assessing the hybridization pattern in metaphase chromosomes of interphase lymphocytes from peripheral blood.

Performance characteristic	Outcome
Theoretical specificity	Mapped on chromosome 7, locus p11.2 and the centromeric region p11.1-q11.1
Practical specificity	100%

## Limitations of Procedure

- i) The REMBRANDT® LSI 7p11.2/CEP7-FISH assay is solely applicable for the detection of the 7p11.2 locus and the centromeric region of chromosome 7, which may be present in cell preparations (cytological specimen i.e. interphase lymphocytes from peripheral blood samples).
- ii) Either human tissue sections or human cytological preparations may be used. Samples must be fixed in buffered formalin or alcohol. In tissue sections are required, the sections should be prepared in a 4 µm thickness. Furthermore, the tissues should be glued to the glass slides with a bio-adhesive (e.g. organ silane), dried at room temperature, subsequently dried at 37 °C overnight and lastly completely deparaffinized in xylene and alcohol series and air dried.
- iii) Cytological specimen should be prepared as required by the user, fixed with cytological fixation agent, rinsed in distilled water prior to the ISH procedure and air dried.
- iv) Many factors can influence the performance of the ISH procedure. Failure in detection can be due to i.e. improper sampling, handling, the time lapse between tissue removal and fixation, the size of the tissue specimen in the fixation medium, the fixation time, processing fixed tissue, the thickness of the section, the bio-adhesive on the slide, deparaffinisation procedure, incubation times, proteolytic pre-treatment, detection reagents, incubation temperatures and interpretation of results.
- v) The performance of the ISH procedure is also affected by the sensitivity of the method and the presence of the locus 7p11.2 and the centromeric region of chromosome 7. In case the limit of the sensitivity is reached a false negative reaction may be the result.
- viii) Therapeutic considerations based on the result of this test alone should not be taken. Results should be verified by other traditional diagnostic methods such as but not limited to clinical history, symptoms, as well as morphological data.
- ix) The medical profession should be aware of risks and factors influencing the fluorescent signal intensity while interpreting the test result. Microscopy settings might influence the signal intensity and/or interpretation.
- x) Laboratory personnel performing the test should be trained and knowledgeable to be able to interpret the test results.

## Storage and handling

Store kit and its contents at 2-8°C. Store the dissolved and aliquoted reagents at recommended temperatures. When used and stored as indicated, the kit is stable until the expiry date printed on the box.

Product	Product number	Storage conditions
LSI 7p11.2/CEP7 Probe orange	C816P.2030	2-8 °C

/green detection			
Pepsin powder	R011R.0000	Powder: 2-25 °C, ambient temperature	
Pepsin diluent	R018R.0000	Dissolved: -20 °C Concentrated solution and diluted: 2-25 °C, ambient temperature	
PanWash 4, 25X SSC	R025R.0000	Concentrated solution and diluted: 2-25 °C, ambient temperature	
Fluorescent mounting medium	Z000R.0050	2-8 °C	



## Hazard statements

H315 - Causes skin irritation  
H319 - Causes serious eye irritation  
H351 - Suspected of causing cancer  
H360D - May damage the unborn child  
H373 - May cause damage to organs through prolonged or repeated exposure

## Precautionary Statements

P202 - Do not handle until all safety precautions have been read and understood  
P280 - Wear protective gloves/protective clothing/eye protection/face protection  
P302 + P352 - IF ON SKIN: Wash with plenty of water and soap  
P305 + P351 + P338 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing  
P308 + P313 - IF exposed or concerned: Get medical advice/attention  
P362 + P364 - Take off contaminated clothing and wash it before reuse  
P405 - Store locked up

## Additional information

### Product in combination with other devices

The REMBRANDT® DNA probes are intended for stand-alone usage. The in vitro diagnostic is intended to be used in combination with standard cytological preparation methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature and incubation time control(s), proteolytic-, detection- and other reagents (not supplied with this reagent) and a microscope. The combination has been tested and validated. Since the standard cytological preparation methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature controls, incubation time control(s) and other not supplied reagents such as but not limited to proteolytic reagents, detection reagents and a microscope is not combined with the device as a

product, conformity with the essential requirements is not applicable. Assay validation criteria are mentioned in 'Interpretation of the Results' and are also depending on clinical state of the sample, which may influence the validation criteria.

For additional information regarding the REMBRANDT® assays, a manual is included which specifies the following subjects:

- Controls
- Materials required but not included
- Storage and shelf-life
- Performance precautions
- Preparations of reagents
- Specimen collection
- Quality control
- Trouble shooting guide

## Technical assistance

For technical assistance regarding the products performance, please contact [info@panpath.nl](mailto:info@panpath.nl) or call +31 495499090. Visit our website for reprints of datasheets or additional documentation. [www.panpath.nl](http://www.panpath.nl)

## Literature list



- Arsham, M. S., Barch, M. J., & Lawce, H. J. (2017). *The AGT Cytogenetics Laboratory Manual The AGT Cytogenetics Laboratory Manual Edited by* (Vol. 4).
- Yoo, S. B., Lee, H. J., Park, J. O., Choe, G., Chung, D. H., Seo, J. W., & Chung, J. H. (2010). Reliability of chromogenic in situ hybridization for epidermal growth factor receptor gene copy number detection in non-small-cell lung carcinomas: A comparison with fluorescence in situ hybridization study. *Lung Cancer*, 67(3), 301–305. <https://doi.org/10.1016/j.lungcan.2009.05.002>



**DATA SHEET-V1**  
**REMBRANDT® LSI 7p11.2/CEP7-ISH**  
**DETECTION**  
**RESEARCH USE ONLY (RUO)**

**RUO**

**PanPath**

<b>Ref</b>	<b>C816K.0199.05</b>		5 T
	<b>C816K.0199.10</b>		10 T

**Intended use**


- I. The REMBRANDT® LSI 7p11.2/CEP7-ISH assay is intended for the detection of the 7p11.2 locus, compared to the centromeric region of chromosome 7 by means of *in situ* hybridization.
- II. The REMBRANDT® LSI 7p11.2/CEP7-ISH detection assay is intended for the detection of the 7p11.2 locus, compared to the centromeric region of chromosome 7 in fixed cells. A clinical diagnosis should not be established based on the performance of this test.
- III. The intended users are qualified laboratory employees in cytology and/or pathology. The product is intended for professional use.

**Clinical relevance**

On the chromosome 7, locus p11.2, the gene for the Epidermal Growth Factor Receptor (EGFR), also known as HER1, is a tyrosine kinase receptor type 1 is located. EGFR is able to interact with epidermal growth factor proteins which result in proliferation. Increased activity of EGFR can result in proliferative diseases such as non-small-cell lung carcinoma (80-85% of all lung cancers). Moreover, EGFR amplifications have been associated with lung adenocarcinoma, glioblastoma, colon adenocarcinoma and breast carcinoma (Yoo et al., 2010).

**Probe specification**

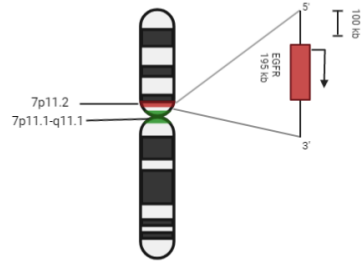

The LSI 7p11.2/CEP7 probes set consists of a 600 kb probe detecting the 7p11.2 locus and a 0.68 kb centromeric probe detecting the centromeric region of chromosome 7. The centromeric region is conjugated to biotin and the locus is conjugated to digoxigenin. The LSI 7p11.2 probe is able to completely cover the EGFR gene with flanking sequences on the 5' and 3' of the gene for signal enhancement. The EGFR amplification probes are pre-mixed in a hybridization mixture (formamide, dextran sulphate and SSC) and are ready to use solutions.



**Test principle**

In an *in situ* hybridization assay, a double stranded DNA probe labelled with a hapten is used. The labelled DNA probe is diluted in a hybridization mixture. The hybridization mixture containing the DNA probe is added to the specimen. A co-denaturation will ensure that the genomic DNA and the probe DNA become single stranded. After denaturation, the probe DNA is able to hybridize to its complementary target sequences in the cells. In the REMBRANDT® LSI 7p11.2/CEP7-ISH assay, the haptens are attached to the probe and the signals can be visualized after detection by corresponding antibodies by fluorescent or brightfield microscopy.

**Reagents provided**

<b>Product name</b>	<b>Product number</b>	<b>Amount</b>
Labelled probe (depending on label and size choice)		
● LSI 7p11.2/CEP7-ISH amplification probes biotin/digoxigenin detection	C816P.0199.05	 5 T
● LSI 7p11.2/CEP7-ISH amplification probes biotin/digoxigenin detection	C816P.0199.10	 10 T
Pepsin powder	R011R.0000	1 g
Pepsin diluent	R018R.0000	15 ml
PanWash 4, 25X SSC	R025R.0000	15 ml

## Assay procedure

REMBRANDT® LSI 7p11.2/CEP7-ISH detection assay procedure for cytological specimen.

- I. Incubate slides in pre-heated proteolytic work solution (prepare according to section 1.9 of Manual-FISH) (R011R.000 + R018R.000) at 37 °C (100 µg/ml) for 15 minutes followed by a brief rinsing in 0.01M HCl (1x 2 minutes) and subsequent rinses in PBS (2x 1 minute)
- II. Flush wash slides in deionised water, followed by dehydration in graded ethanol series (ethanol 70%, 96%, 96%, 100%, 100%) 1 minute each and air-dry slides for 15 minutes

**Do not treat more than 5 slides at the same time, because the temperature of the pre-heated solutions may drop dramatically, thus causing incomplete pre-treatment. Additionally, allow the slides to air-dry as recommended; otherwise sections will be lost.**

- III. Homogenize probe solution (C816P.0199.YY) a spin briefly. Apply 15 µl of probe solution to each specimen. Cover all specimens with a cover slip (avoid air bubbles). Denature slides on a 80 °C hotplate or other heating device for 3 minutes

**Work in a pre-set order to ensure that all slides have been incubated at 80 °C for the exact same time. Do not denature more than 5 slides at the same time, the temperature of the heating device may drop dramatically, thus causing incomplete denaturation.**

- IV. Transfer the slides into a moist environment and incubate for 16 hours at 37 °C.
- V. Remove coverslips by soaking the slides in PBS at room temperature
- VI. Incubate the slides in diluted, pre-heated PanWash 4 (R025R.000) (prepare according to section 1.9 of Manual-FISH)

**Do not incubate more than 5 slides at the same time in PanWash 4, the temperature of the PanWash 4 may drop dramatically, causing wrong stringency conditions.**

- VII. Appropriate detection system should be evaluated by the end-user. Recommended detection systems are listed below





Digoxigenin detection	Biotin detection
R003R.0000 Sheep aDig-AP conjugate	R041R.0000 Goat aBio-AP Fab conjugate
R004R.0000 Sheep aDig-HRP conjugate	R042R.0000 Goat aBio-HRP Fab conjugate

## Interpretation of results

Hybridization of the LSI 7p11.2/CEP7 probe is viewed using a fluorescence or bright field microscope equipped with appropriate excitation and emission filters. Allowing visualization of ISH signals concentrated at the 7p11.2 locus, and the centromeric region of chromosome 7. The enumeration of the locus 7p11.2 is conducted by microscopic examination of interphase nuclei.

The assay procedure enables visual enumeration of the 7p11.2 locus, compared to the centromeric region of chromosome 7 within the nuclei. Enumerate the fluorescent signals in the interphase nucleus using a 40X or 63X magnification. Objectives with higher magnification (eg, 63X or 100X) should be used to verify or resolve questions about split or diffused signals. Enumerate at least 100 nuclei per slide for accurate analysis. Enumerate the fluorescent signals in the interphase nucleus using a 40X or 63X magnification. Objectives with higher magnification (eg, 63X or 100X) should be used to verify or resolve questions about split or diffused signals. Enumerate at least 100 nuclei per slide for accurate analysis.

- Two signals in close proximity and approximately the same sizes but not connected by a visible link are counted as 2 signals.
- Count a diffuse signal as 1 signal if diffusion of the signal is contiguous and within an acceptable boundary.
- Two small signals connected by a visible link are counted as 1 signal.
- Enumerate the number of nuclei with 0, 1, 2, 3, 4, or >4 signals. Count nuclei with 0 signals only if there are other nuclei with at least 1 signal present in the field of view. If the accuracy of the enumeration is in doubt, repeat the enumeration in another area of the slide.
- Do not enumerate nuclei with uncertain signals

- 1  Do not count, overlapping nuclei
- 2  Count as two signals. 1 compact and 1 diffused signal
- 3  Count as two signals. 1 split signal and 1 diffused signal
- 4  Count as 3 signals

## Performance characteristics

### Analytical Sensitivity and Specificity

The LSI 7p11.2/CEP7-ISH detection assay was analytically validated for LSI 7p11.2/CEP7-FISH detection. The results of the direct fluorescent assay are shown. However, for the REMBRANDT® LSI 7p11.2/CEP7-ISH detection assay, the detection system may influence the performance characteristics and LSI 7p11.2/CEP7-ISH detection assay in combination with different detection systems should be evaluated carefully by the end-user.

### Analytical sensitivity

The analytical sensitivity was determined in three levels. The normal cut-off percentage was determined based on assessment of 200 individual nuclei in two samples of healthy interphase lymphocytes from peripheral blood. The beta inversion was used to determine the percentage of normal-cut off. For the noise-to-signal percentage, the noise and signal values were determined for 100 signals in interphase lymphocytes from peripheral blood of two independent samples. The differences between noise and signal were evaluated using a 95% confidence interval. For the hybridization efficiency, 200 individual nuclei were assessed for the presence of ISH signals.

Performance characteristic	Outcome
Normal cut-off percentage	10.9%
Noise-to-signal cut-off percentage	14.8%
Hybridization efficiency	98.5%

### Analytical specificity

The analytical specificity was determined in two levels. The theoretical specificity was determined by sequencing analysis of the probe DNA and mapping on Hg38. The practical specificity was determined by assessing the hybridization pattern in metaphase chromosomes of interphase lymphocytes from peripheral blood.

Performance characteristic	Outcome
Theoretical specificity	Mapped on chromosome 7, p11.2 and the centromeric region p11.1-q11.1
Practical specificity	100%

## Limitations of Procedure

- i) The REMBRANDT® LSI 7p11.2/CEP7-ISH assay is solely applicable for the detection of the locus 7p11.2 and the centromeric region of the human chromosome 7, which may be present in cell preparations (cytological specimen i.e. interphase lymphocytes from peripheral blood samples).
- ii) Either human tissue sections or human cytological preparations may be used. Samples must be fixed in buffered formalin or alcohol. In tissue sections are required, the sections should be prepared in a 4 µm thickness. Furthermore, the tissues should be glued to the glass slides with a bio-adhesive (e.g. organ silane), dried at room temperature, subsequently dried at 37 °C overnight and lastly completely deparaffinized in xylene and alcohol series and air dried.
- iii) Cytological specimen should be prepared as required by the user, fixed with cytological fixation agent, rinsed in distilled water prior to the ISH procedure and air dried.
- iv) Many factors can influence the performance of the ISH procedure. Failure in detection can be due to i.e. improper sampling, handling, the time lapse between tissue removal and fixation, the size of the tissue specimen in the fixation medium, the fixation time, processing fixed tissue, the thickness of the section, the bio-adhesive on the slide, deparaffinisation procedure, incubation times, proteolytic pre-treatment, detection reagents, incubation temperatures and interpretation of results.
- v) The performance of the ISH procedure is also affected by the sensitivity of the method and the presence of the locus 7p11.2 and the centromeric region of chromosome 7. In case the limit of the sensitivity is reached a false negative reaction may be the result.
- vi) The REMBRANDT® LSI 7p11.2/CEP7-ISH assay results should not be relied on in case the sampling, sampling method, sample quality, sample preparation, reagents used, controls and procedure followed are not optimal or as described the working protocols.
- vii) The medical profession should be aware of risks and factors influencing the fluorescent signal intensity while interpreting the test result. Microscopy settings might influence the signal intensity and/or interpretation.
- viii) Laboratory personnel performing the test should be trained and knowledgeable to be able to interpret the test results.

## Storage and handling

Store kit and its contents at 2-8°C. Store the dissolved and aliquoted reagents at recommended temperatures. When used and stored as indicated, the kit is stable until the expiry date printed on the box.

Product	Product number	Storage conditions
LSI 7p11.2/CEP7-	C816P.XXXX	2-8 °C

ISH probes biotin/digoxigenin detection PanWash 4, 25X SSC	R025R.0000	Concentrated solution and diluted: 2-25° C, ambient temperature
Pepsin powder	R011R.0000	Powder: 2-25° C, ambient temperature
Pepsin diluent	R018R.0000	Dissolved: -20° C Concentrated solution and diluted: 2-25° C, ambient temperature



## Hazard statements

H315 - Causes skin irritation  
H319 - Causes serious eye irritation  
H351 - Suspected of causing cancer  
H360D - May damage the unborn child  
H373 - May cause damage to organs through prolonged or repeated exposure

## Precautionary Statements

P202 - Do not handle until all safety precautions have been read and understood  
P280 - Wear protective gloves/protective clothing/eye protection/face protection  
P302 + P352 - IF ON SKIN: Wash with plenty of water and soap  
P305 + P351 + P338 - IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lenses, if present and easy to do. Continue rinsing  
P308 + P313 - IF exposed or concerned: Get medical advice/attention  
P362 + P364 - Take off contaminated clothing and wash it before reuse  
P405 - Store locked up

## Additional information

### Product in combination with other devices

The REMBRANDT® DNA probes are intended for stand-alone usage. The in vitro diagnostic is intended to be used in combination with standard cytological preparation methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature and incubation time control(s), proteolytic-, detection- and other reagents (not supplied with this reagent) and a microscope. The combination has been tested and validated. Since the standard formalin fixed, paraffin embedded tissue blocks, standard tissue freezing, tissue sectioning (microtome), standard cytological preparation methods, hot plate(s), stove(s), incubation device(s), water bath(s), temperature controls,

incubation time control(s) and other not supplied reagents such as but not limited to proteolytic reagents, detection reagents and a microscope is not combined with the device as a product, conformity with the essential requirements is not applicable. Assay validation criteria are mentioned in 'Interpretation of the Results' and are also depending on the target load, which may influence the validation criteria.

For additional information regarding the REMBRANDT® assays, a manual is included which specifies the following subjects:

- Controls
- Materials required but not included
- Storage and shelf-life
- Performance precautions
- Preparations of reagents
- Specimen collection
- Quality control
- Trouble shooting guide

## Technical assistance

For technical assistance regarding the products performance, please contact [info@panpath.nl](mailto:info@panpath.nl) or call +31 495499090. Visit our website for reprints of datasheets or additional documentation. [www.panpath.nl](http://www.panpath.nl)

## Literature list

- Arsham, M. S., Barch, M. J., & Lawce, H. J. (2017). *The AGT Cytogenetics Laboratory Manual The AGT Cytogenetics Laboratory Manual Edited by* (Vol. 4).
- Yoo, S. B., Lee, H. J., Park, J. O., Choe, G., Chung, D. H., Seo, J. W., & Chung, J. H. (2010). Reliability of chromogenic in situ hybridization for epidermal growth factor receptor gene copy number detection in non-small-cell lung carcinomas: A comparison with fluorescence in situ hybridization study. *Lung Cancer*, 67(3), 301–305. <https://doi.org/10.1016/j.lungcan.2009.05.002>